


Differences Between the pHoenix XL and the Older pHoenix Meter

The pHoenix XL meter does not use Level 1 and Level 2 calibrations.

- The older pHoenix meter process called a Level 1 calibration is now a daily verification or calibration at 14.0 mS and 7.0 pH.
- The older pHoenix meter process called a Level 2 calibration is now the extended range calibrations, to be performed monthly or as needed.

The pHoenix XL **DOES NOT** use the UP and DOWN arrows to manually adjust the calibration.

- The new process is to select the calibration reference value from the menus, expose the meter to the calibration solution, and CAL it, causing the new meter to instantly change its calibration.

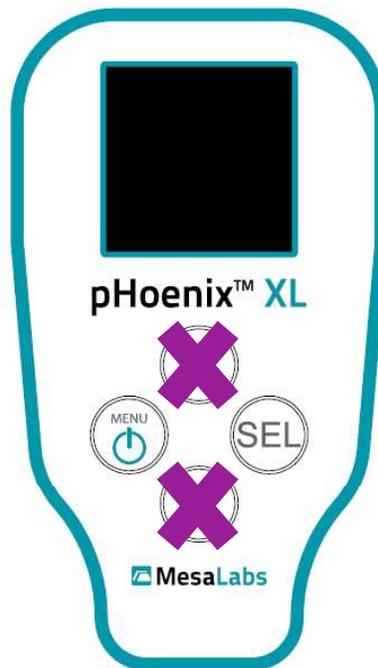

**DO NOT USE UP /
DOWN ARROWS
FOR CALIBRATION
OR MEASUREMENT**

The new pHoenix XL performs calibration range checking.

- If the measured value during calibration is significantly different from the menu selection, the new meter will indicate an "Out of Range" condition.